

LG ELECTRONICS CO., LTD.

TEST REPORT

SCOPE OF WORKS

EVALUATION OF STERILIZATION EFFICIENCY OF DISINFECTION ROBOT USING UV-C LIGHT DEVICES

REPORT NUMBER RT21E-S0013

ISSUE DATE 02-APR-2021

PAGES

30

DOCUMENT CONTROL NUMBER

ISTC-QP-FM-17-03-E1 Rev.1 © 2017 INTERTEK





Report No.: RT21E-S0013 Date: APR 02, 2021

OBJECTIVE

The purpose of the testing is:

To define test conditions and evaluate the efficacy of microorganisms inactivation on the surface materials by a disinfection robot using UV-C light devices.

HYPOTHESIS

Staphylococcus aureus & Salmonella on stainless steel exposed to UVC will be decreased 99.999%. Staphylococcus aureus & Salmonella on glass exposed to UVC will be decreased 99.999%. Staphylococcus aureus & Klebsiella pneumoniae on fabric exposed to UVC will be decreased 99.999%.

CONCLUSION

Based on the data collected, the Hypothesis is accepted:

Staphylococcus aureus on stainless steel & glass exposed to UVC lamp at a distance of 1 M can decreased 99.999 % at more than 140 seconds.

Salmonella on stainless steel & glass exposed to UVC lamp at a distance of 1 M can decreased 99.999 % at more than 160 seconds.

Staphylococcus aureus & Klebsiella pneumoniae on fabric exposed to UVC lamp at a distance of 1 M can decreased 99.999 % at more than 140 seconds.

 Rody Ju
 Bo Park

 ENGINEER
 REVIEWER

 CONDUCTED BY
 LG ELECTRONICS INC.

 PERFORMED BY
 INTERTEK TESTING SERVICES KOREA LTD.

 PERIOD OF TEST
 08 MAR 2021 ~ 02 APR 2021

 DATE OF ISSUE
 02 APR 2021

Except where explicitly agreed in writing, all work and services performed by Intertek is subject to our standard Terms and Conditions which can be obtained at our website: http://www.intertek.com/terms/. Intertek's responsibility and liability are limited to the terms and conditions of the agreement. This report is made solely on the basis of your instructions and / or information and materials supplied by you and provide no warranty on the tested sample(s) be truly representative of the sample source. The report is not intended to be a recommendation for any particular course of action, you are responsible for acting as you see fit on the basis of the report results. Intertek is under no obligation to refer to or report upon any facts or circumstances which are outside the specific instructions received and accepts no responsibility to any parties whatsoever, following the issue of the report, for any matters arising outside the agreed scope of the works. This report does not discharge or release you from your legal obligations and duties to any other person. You are the only one authorized to permit copying or distribution of this report (and then only in its entirety). Any such third parties to whom this report may be circulated rely on the content of the report solely at their own risk. This report shall not be reproduced, except in full.

Telephone: 82-6-090-9615 Facsimile: 82-3-409-0505 www.intertek.com

Date: APR. 02, 2021

SECTION 1

INDEX

SECTION NAMES	PAGE
Objective	4
Parameters	4
Product/Model Description	5
Sample acquisition	5
Hypothesis	5
Equipment	6
Technical staff	6
Test procedure	7-10
Test result	11-28
Conclusion	29
Appendix I. Photo of model	30

SECTION 2

OBJECTIVE

The purpose of the testing is:

To define test conditions and evaluate the efficacy of microorganisms inactivation on the surface materials by a disinfection robot using UV-C light devices.

SECTION 3

PARAMETERS

The following parameters are controlled

VALUE	DESCRIPTION	UNITS	METHOD
23 ± 5	Test room temperature	°C	Data logger
65 ± 20	Test room humidity	% R.H.	Data logger
35-37	Incubated Temperature	°C	Data logger

The following parameters are monitored

VALUE	DESCRIPTION	UNITS	METHOD
23 ± 5	Test room temperature	°C	Data logger
65 ± 20	Test room humidity	% R.H.	Data logger
35-37	Incubated Temperature	°C	Data logger

SECTION 4

PRODUCT/MODEL DESCRIPTION

PRODUCT INFORMATION : LG DISINFECTING ROBOT

MODEL :

Note :

SECTION 5 SAMPLE ACQUISITION

Sample(s) was supplied by the applicant:

SAMPLE #	DESCRIPTION	MODEL	PURCHASE LOCATION	DATE	CONDITION
1	Disinfection robot	_	Prepared by LG	2021.2	Packaged and undamaged
2	UV Lamp	Philips TUV 36W SLV/6	Prepared by LG	2021.2	Packaged and undamaged

SECTION 6

HYPOTHESIS

Staphylococcus aureus & Salmonella on stainless steel exposed to UVC will be decreased 99.999%. Staphylococcus aureus & Salmonella on glass exposed to UVC will be decreased 99.999%. Staphylococcus aureus & Klebsiella pneumoniae on fabric exposed to UVC will be decreased 99.999%.

Date: APR. 02, 2021

SECTION 7

EQUIPMENT LIST

#	EQUIPMENT DESCRIPTION	MANUFACTURER'S NAME / MODEL # / SERIAL #	INTERTEK ASSET #	CALIBRATION DATE	CALIBRATION DUE	RANGE USED			
1	Auto clave	JEIOTECH / ST-105G / 1A035183	ISTK-78-00	2020.04.24	2021.04.23	121 °C			
2	Incubator	JEIOTECH / 1L-11 / W070283	ISTK-21-06	2020.08.10	2021.08.10	0 ~ 60 °C			
3	Thermometer	NONE/ JB-913 / TEMPNO.11591	ISTC-64-05	2020.04.27	2021.04.27	10 ~ 30 °C			
4	hydrometer	NONE/ JB-913 / TEMPNO.11591	ISTC-64-05	2020.04.27	2021.04.27	40 ~ 80 %			
5	Pipet (1000)	Biohit / 15582461 /AP-40	ISTC-APM-04	2020.08.20	2021.08.20	100 ~ 1000 uL			
6	Pipet (10)	Biohit / 12527456 /AP-22	ISTC-APM-04	2020.11.10	2021.11.10	10 ~ 100 uL			
7	Balance	AND/CB-2000/H16-02955	ISTK-01-07	2020.08.10	2021.08.10	(0 ~ 2000) g			
8	Clean bench	SEOJIN / - / -	ISTK-23-01	-	-	-			
9	Colony counter	Hwashin / 350CL / -	ISTK-48-01	-	-	-			
Note: Th	Note: The equipment measurement uncertainty is stated in the Test Procedure.								

SECTION 8

TECHNICAL STAFF

#	Staff Name	Area of Expertise				
1	Ej Kim	Technician / Intertek Testing Korea Ltd.				
2	Kenneth Lee	Sr.Engineer / Intertek Testing Korea Ltd.				
3	Rody Ju	Technical Manager / Intertek Testing Korea Ltd.				
4	Bo Park	Laboratory Director / Intertek Testing Korea Ltd.				
Note: Complete training records for staff are available upon request						

Testing was conducted at:

Intertek Testing Services Korea Ltd. 4/F, A-JU Digital Tower, 7, Achasan-ro 5 –gil, Seongdong-gu, Seoul, Korea

Date: APR. 02, 2021


SECTION 9

TEST PROCEDURE

1. Test Set up :

Items		Requirement	Condition	
Electrical Supply	Voltage	(220 ± 10)	(220 ± 10)	
	Frequency	(60 ± 10) Hz	(60 ± 10) Hz	
Ambient Temperature		(25 ± 3) °C	(25 ± 3) °C	
Ambient humidity		(40 ± 10) % R.H.	(40 ± 10) % R.H.	

2. Test Condition :

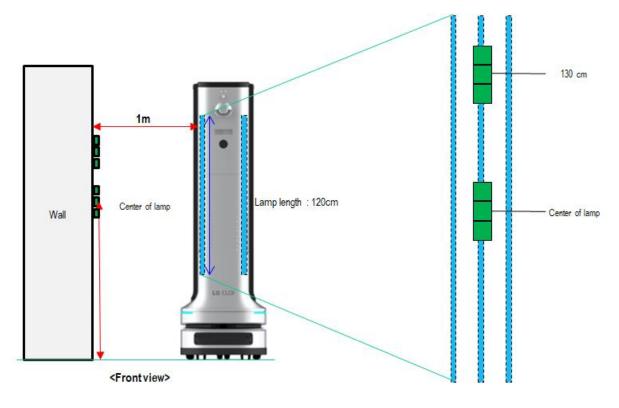

<side view>

3. Sample Description

	Photocatalytic specimens				
Туре	UV Lamp (Philips TUV 36W SLV/6)				
Size	Length : 120mm				
Shape	cylinder				
Photo					

4. Microorganisms

Bacteria Species	Strain Number
Staphylococcus aureus	ATCC 6538
Klebsiella pneumoniae	ATCC 4352
Salmonella enteritidis	ATCC 12021

5. Reagents

Name	Manufacturer	Product No	LOT No	Expiry date	Contents
1 X PBS buffer	gibco	70011-044	2193136	22.09.30	
Tryptic Soy Agar	Difco	236950	0244908	25.07.31	
Tryptic Soy Broth	Difco	211825	9065918	24. 01. 31	

6. Test method

6.1. Preparation of test

- 6.1.1 Disconnect 1 ul of the strains cultured on TSA using a loop, and inoculate it in 100 ml of TSB.
- 6.1.2 Incubate in a 37 °C water bath so that the OD value is between 0.8 and 1.0 in the 600 nm wavelength.
- 6.1.3 Using Standard curve data dilute the number of bacteria to $1.0^{-10.0} \times 10^{7}$ CFU/mL.
- 6.1.4 Put the specimen on an empty Petri dish and inoculate it with 10 ul of the 6.1.3 solution.

On 6 stainless steel & glass samples, inoculate Staphylococcus aureus, Salmonella enteritidis.

On 6 fabric samples, inoculate *Staphylococcus aureus, Klebsiella pneumoniae*.

In this case, Positive control and Negative control (D.W), respectively, are prepared and placed for the same time as the subsequent procedure.

6.1.5 Cover the petri dish lid diagonally and dry it naturally in the clean bench for 30 minutes. At this time, air is allowed to flow for drying.

6.2 Operating of Disinfection robot

The UV is radiated at the distance-time according to the test conditions.

- 6.2.1 Attach the specimen on the wall so that UV can be easily emitted.
- 6.2.2 Turn on the Lamp. (Cover the Lamp)
- 6.2.3 After the light source stabilizes, Remove the cover and Radiate with a UVC lamp for 60 seconds at a distance of 1 M away.
- 6.2.4 In the same way, repeat the test again for 80s, 100s, 120s and 140s.
- 6.2.5 Change every lamp to another batch.
- 6.2.6 Triplicate test complete

Date: APR. 02, 2021

6.3 Extraction of bacteria from sample specimen

6.3.1 Swab three times per specimen recovered and put it in a 50 mL tube containing 10mL of 1X PBS buffer.

In the case of fabric, it is placed directly into a 50 mL conical tube containing 10mL of 1X PBS buffer without Swab.

6.3.2 Voltex more than 5 minutes.

6.4 The method of examination

- 6.4.1 Get 1 mL of Solution and put in an empty Petri dish, and then add 20 mL of TSA medium stored at 45-50°C.
- 6.4.2 All plates incubate for (48 \pm 4) hours at 37 °C.
- 2.6.3 After incubation, the plates enumerated.

6.5 Calculation of result

- 6.5.1 Percent reduction = $[(a-b)/a] \times 100$
- a : the microorganism number of Positive control
- b : the microorganism number of after UV radiation.

Date: APR. 02, 2021

SECTION 10

TEST RESULT

Stainless steel - *Staphylococcus aureus*

			130 cm			100 cm	
Repeat #1	Sample	Result	Average	Reduction rate (%)	Result	Average	Reduction rate (%)
Positive	Control 1	2.2 × 10 ⁶	2.1 × 105		2.2 × 10 ⁶		
control	Control 2	2.0 × 10 ⁶	2.1 × 10 ⁶	2.1 × 10° -	2.0 × 10 ⁶	2.1 × 10 ⁶	-
	Sample 1	2.6 × 10 ³			4.8 × 10 ²		
60s	Sample 2	5.5 × 10²	1.5 × 10 ³	99.928	7.4 × 10 ²	7.7 × 10²	99.963
	Sample 3	1.3 × 10 ³			1.1 × 10 ³		
	Sample 1	5.5 × 10 ²			1.8 × 10 ²		
80s	Sample 2	2.3 × 10 ²	3.7 × 10 ²	99.982	2.0 × 10 ¹	7.0 × 10 ¹	99.996
	Sample 3	3.2 × 10 ²			1.0 × 10 ¹		
	Sample 1	6.0 × 10 ¹			6.0 × 10 ¹		
100s	Sample 2	7.0 × 10 ¹	6.0 × 10 ¹	99.997	3.5 × 10 ²	1.5 × 10²	99.993
	Sample 3	5.0 × 10 ¹			2.5 × 10 ¹		
	Control 1	1.4 × 10 ⁶	1.2 105		1.4 × 10 ⁶	1.2 105	
	Control 2	1.1 × 10 ⁶	1.2 × 10 ⁶	-	1.1 × 10 ⁶	1.2 × 10 ⁶	-
120s	Sample 1	5.0 × 10 ¹			1.5 × 10 ¹		
	Sample 2	2.0 × 10 ¹	3.0 × 10 ¹	99.997	2.0 × 10 ¹	1.3 × 10 ¹	99.998
	Sample 3	2.5 × 10 ¹			5.0 × 10 ⁰		
	Sample 1	0			0		
140s	Sample 2	0	0	99.999	0	0	99.999
	Sample 3	0			0		

Date: APR. 02, 2021

Stainless steel - Staphylococcus aureus

			130 cm			100 cm	
Repeat #2	Sample	Result	Average	Reduction rate (%)	Result	Average	Reduction rate (%)
Positive	Control 1	2.0 × 10 ⁶	1 7 × 105		2.0 × 10 ⁶	1 7 × 105	
control	Control 2	1.5 × 10 ⁶	1.7 × 10 ⁶	-	1.5 × 10 ⁶	1.7 × 10 ⁶	-
	Sample 1	4.1 × 10 ²			1.9 × 10 ²		
60s	Sample 2	3.8 × 10 ²	3.4 × 10 ²	99.980	2.5 × 10 ¹	8.5 × 10 ¹	99.995
	Sample 3	2.4 × 10 ²			4.5 × 10 ¹		
	Sample 1	4.0 × 10 ¹			2.0 × 10 ¹		
80s	Sample 2	2.0 × 10 ¹	4.0 × 10 ¹	99.997	4.0×10^{1}	4.0×10^{1}	99.997
	Sample 3	6.5 × 10 ¹	101		7.0 × 10 ¹		
	Sample 1	9.0 × 10 ¹			3.0 × 10 ¹		
100s	Sample 2	1.4 × 10 ²	9.8×10^{1}	99.994	5.0 × 10 ⁰	3.3 × 10 ¹	99.998
	Sample 3	7.0 × 10 ¹			6.5 × 10 ¹		
	Control 1	9.6 × 10 ⁵	9.7 × 10 ⁵		9.6 × 10 ⁵	9.7 × 10 ⁵	
	Control 2	9.7 × 10⁵	9.7 × 103	-	9.7 × 10⁵	9.7 × 103	-
120s	Sample 1	1.5 × 10 ¹			5.0×10^{0}		
	Sample 2	0	5.0 × 10 ⁰	99.999	2.0 × 10 ¹	1.0×10^{1}	99.999
	Sample 3	0			5.0 × 10º		
	Sample 1	5.0×10^{0}			0		
140s	Sample 2	2.0 × 10 ¹	8.0×10^{0}	99.999	1.5 × 10 ¹	5.0×10^{0}	99.999
	Sample 3	0			0		

Date: APR. 02, 2021

Stainless steel - Staphylococcus aureus

			130 cm			100 cm	
Repeat #3	Sample	Result	Average	Reduction rate (%)	Result	Average	Reduction rate (%)
Positive	Control 1	3.3 × 10 ⁶	2.0.4.105		3.3 × 10 ⁶	2.0	
control	Control 2	2.4 × 10 ⁶	2.9 × 10 ⁶		2.4 × 10 ⁶	2.9 × 10 ⁶	-
	Sample 1	8.0 × 10 ²			4.4×10^{2}		
60s	Sample 2	9.2 × 10 ²	6.2 × 10 ²	99.979	6.0 × 10 ²	5.4 × 10 ²	99.981
	Sample 3	1.5 × 10²			5.7 × 10 ²		
	Sample 1	4.5 × 10 ²			3.5 × 10 ²		
80s	Sample 2	8.7 × 10 ²	5.4 × 10 ²	99.981	8.5 × 10 ¹	3.3 × 10 ²	99.989
	Sample 3	2.9 × 10 ²			5.5 × 10 ²		
	Sample 1	1.0 × 10 ¹			1.5 × 10 ¹		
100s	Sample 2	0	3.7 × 10 ¹	99.998	6.0 × 10 ¹	2.5 × 10 ¹	99.999
	Sample 3	1.0 × 10 ²			0		
	Control 1	3.4 × 10 ⁶			3.4 × 10 ⁶	2 7 405	
	Control 2	2.1 × 10 ⁶	2.7 × 10 ⁶	-	2.1 × 10 ⁶	2.7 × 10 ⁶	-
120s	Sample 1	3.0 × 10 ¹			5.0 × 10 ⁰		
	Sample 2	2.5 × 10 ¹	2.0 × 10 ¹	99.999	1.0 × 10 ¹	1.0×10^{1}	99.999
	Sample 3	5.0×10^{0}			1.5 × 10 ¹		
	Sample 1	1.0 × 10 ¹			1.5 × 10 ¹		
140s	Sample 2	5.0×10^{0}	2.0 × 10 ¹	99.999	0	7.0×10^{0}	99.999
	Sample 3	4.5 × 10 ¹			5.0 × 10 ⁰		

Date: APR. 02, 2021

Stainless steel - Salmonella enteritidis

			130 cm			100 cm	
Repeat #1	Sample	Result	Average	Reduction rate (%)	Result	Average	Reduction rate (%)
Positive	Control 1	7.6 × 10 ⁵			7.6 × 10⁵		
control	Control 2	5.5 × 10 ⁵	6.6 × 10 ⁵	-	5.5 × 10 ⁵	6.6 × 10 ⁵	-
	Sample 1	1.9 × 10 ³			1.8 × 10 ³		
60s	Sample 2	7.7 × 10 ²	1.3 × 10 ³	99.803	1.3 × 10 ³	1.4 × 10 ³	99.788
	Sample 3	1.4 × 10 ³			1.0 × 10 ³		
	Sample 1	1.0 × 10 ³			1.4 × 10 ³		
80s	Sample 2	2.3 × 10 ³	1.5 × 10 ³	99.772	1.0 × 10 ³	1.3 × 10 ³	99.803
	Sample 3	1.4 × 10 ³			1.4 × 10 ³		
	Sample 1	3.0 × 10 ¹			2.5 × 10 ¹		
100s	Sample 2	1.5 × 10 ¹	3.8 × 10 ¹	99.994	5.0 × 10 ¹	4.8×10^{1}	99.993
	Sample 3	7.0 × 10 ¹			7.0 × 10 ¹		
	Control 1	6.7 × 10 ⁵	6.0		6.7 × 10 ⁵		
	Control 2	6.9 × 10 ⁵	6.8 × 10 ⁵	-	6.9 × 10 ⁵	6.8 × 10 ⁵	-
120s	Sample 1	1.5 × 10 ¹			4.5 × 10 ¹		
	Sample 2	6.0 × 10 ¹	3.7 × 10 ¹	99.995	2.5 × 10 ¹	4.0×10^{1}	99.994
	Sample 3	3.5 × 10 ¹			5.0 × 10 ¹		
	Sample 1	1.0 × 10 ²			2.0 × 10 ¹		
140s	Sample 2	8.0 × 10 ¹	6.5 × 10 ¹	99.990	2.5 × 10 ¹	2.7 × 10 ¹	99.995
	Sample 3	1.5 × 10 ¹			3.5 × 10 ¹		
Positive	Control 1	4.7 × 10 ⁵	C 0 ++ 105		4.7 × 10 ⁵	C 0 ++ 10 ⁵	
control	Control 2	7.3 × 10 ⁵	6.0 × 10 ⁵	-	7.3 × 10⁵	6.0 × 10 ⁵	-
	Sample 1	0			0		
160s	Sample 2	0	0	99.999	0	3.0×10^{0}	99.999
	Sample 3	0			1.0 × 10 ¹		
	Sample 1	0			5.0 × 10 ⁰		-
180s	Sample 2	0	2.0 × 10 ⁰	99.999	0	2.0 × 10 ⁰	99.999
	Sample 3	5.0 × 10 ⁰			0		

Date: APR. 02, 2021

Stainless steel - Salmonella enteritidis

			130 cm			100 cm	
Repeat #2	Sample	Result	Average	Reduction rate (%)	Result	Average	Reduction rate (%)
Positive	Control 1	2.9 × 10 ⁵			2.9 × 10 ⁵		
control	Control 2	2.8 × 10 ⁵	2.8 × 10 ⁵	-	2.8 × 10 ⁵	2.8 × 10 ⁵	-
	Sample 1	1.5 × 10 ²			2.0 × 10 ¹		
60s	Sample 2	3.5 × 10 ¹	1.2 × 10 ²	99.957	6.0 × 10 ¹	3.5 × 10 ¹	99.988
	Sample 3	1.6 × 10 ²			2.5 × 10 ¹		
	Sample 1	0			5.0 × 10 ⁰		
80s	Sample 2	0	3.0 × 10 ⁰	99.998	2.5 × 10 ¹	1.5 × 10 ¹	99.995
	Sample 3	1.0 × 10 ¹			1.5 × 10 ¹		
	Sample 1	0			5.0 × 10 ⁰		
100s	Sample 2	5.0 × 10 ⁰	7.0×10^{0}	99.998	0	7.0×10^{0}	99.998
	Sample 3	1.5 × 10 ¹			1.5 × 10 ¹		
	Control 1	8.3 × 10 ⁵	77.405		8.3 × 10 ⁵	7.7 × 10 ⁵	
	Control 2	7.2 × 10 ⁵	7.7 × 10 ⁵	-	7.2 × 10 ⁵		-
120s	Sample 1	3.5 × 10 ¹			2.5 × 10 ¹		
	Sample 2	0	3.3 × 10 ¹	99.996	0	8.0×10^{0}	99.999
	Sample 3	6.5 × 10 ¹			0		
	Sample 1	0			0		
140s	Sample 2	5.0×10^{0}	5.0×10^{0}	99.998	0	0	99.999
	Sample 3	1.0×10^{1}			0		
Positive	Control 1	6.3 × 10 ⁵	6.9 × 10⁵		6.3 × 10 ⁵	6.9 × 10⁵	
control	Control 2	7.4 × 10 ⁵	6.9 × 10 ³	-	7.4 × 10 ⁵	6.9 × 10°	-
	Sample 1	0					
160s	Sample 2	0	0	99.999		2.0 × 10 ⁰	99.999
	Sample 3	0			5.0 × 10 ⁰		
	Sample 1	0			0		-
180s	Sample 2	0	0	99.999	0	0	99.999
	Sample 3	0			0		

Date: APR. 02, 2021

Stainless steel - Salmonella enteritidis

			130 cm			100 cm	
Repeat #3	Sample	Result	Average	Reduction rate (%)	Result	Average	Reduction rate (%)
Positive	Control 1	8.8 × 10 ⁵			8.8 × 10 ⁵		
control	Control 2	5.7 × 10 ⁵	7.3 × 10 ⁵	-	5.7 × 10 ⁵	7.3 × 10 ⁵	-
	Sample 1	4.0 × 10 ¹			2.0 × 10 ¹		
60s	Sample 2	2.0 × 10 ¹	2.5 × 10 ¹	99.997	2.0 × 10 ¹	1.8 × 10 ¹	99.998
	Sample 3	1.5 × 10 ¹			1.5 × 10 ¹		
	Sample 1	1.5 × 10 ¹			3.5 × 10 ¹		
80s	Sample 2	1.0 × 10 ¹	2.2 × 10 ¹	99.997	1.0 × 10 ¹	1.7 × 10 ¹	99.998
	Sample 3	4.0×10^{1}			5.0 × 10 ⁰		
	Sample 1	1.5 × 10 ¹			5.0 × 10 ¹		
100s	Sample 2	1.5 × 10 ¹	1.2 × 10 ¹	99.998	0	1.7 × 10 ¹	99.998
	Sample 3	5.0 × 10 ⁰			0		
	Control 1	5.8 × 10 ⁵	6.2 105		5.8 × 10 ⁵	6.2 × 10 ⁵	
	Control 2	6.5 × 10 ⁵	6.2 × 10 ⁵	-	6.5 × 10 ⁵		-
120s	Sample 1	5.0 × 10 ⁰	2.0×10^{0}	99.999	2.0 × 10 ¹	7.0 × 10 ⁰	
	Sample 2	0			0		99.998
	Sample 3	0			0		
	Sample 1	5.0×10^{0}			0		
140s	Sample 2	5.0×10^{0}	7.0×10^{0}	99.999	0	2.0 × 10 ⁰	99.999
	Sample 3	1.0×10^{1}			5.0×10^{0}		
Positive	Control 1	5.6 × 10 ⁵	5 7 405		5.6 × 10 ⁵	5 7 405	
control	Control 2	5.8 × 10 ⁵	5.7 × 10 ⁵	-	5.8 × 10 ⁵	5.7 × 10 ⁵	-
	Sample 1	0			0		
160s	Sample 2	5.0 × 10 ⁰	3.0×10^{0}	99.999	0	5.0 × 10 ⁰	99.999
	Sample 3	5.0 × 10 ⁰			1.5 × 10 ¹		
	Sample 1	0			0		
180s	Sample 2	0	0	99.999	5.0 × 10 ⁰	2.0 × 10 ⁰	99.999
	Sample 3	0			0		

Glass - Staphylococcus aureus

			130 cm			100 cm	
Repeat #1	Sample	Result	Average	Reduction rate (%)	Result	Average	Reduction rate (%)
Positive	Control 1	1.5 × 10 ⁶	1 4 × 105		1.5 × 10 ⁶	1 4 × 106	
control	Control 2	1.3 × 10 ⁶	1.4 × 10 ⁶		1.3 × 10 ⁶	1.4 × 10 ⁶	-
	Sample 1	1.5 × 10 ²			2.1 × 10 ²		
60s	Sample 2	2.2 × 10 ²	2.2 × 10 ²	99.984	4.3 × 10 ²	3.2 × 10 ²	99.977
	Sample 3	3.0 × 10 ²			3.4 × 10 ²		
	Sample 1	1.9 × 10 ²			4.8 × 10 ²		
80s	Sample 2	1.5 × 10 ²	1.7 × 10 ²	99.988	3.0 × 10 ²	3.6 × 10 ²	99.974
	Sample 3	1.8 × 10 ²			3.1 × 10 ²		
	Sample 1	5.0 × 10 ⁰			5.0×10^{0}		
100s	Sample 2	0	2.0 × 10 ⁰	99.999	1.5 × 10 ¹	7.0 × 10 ⁰	99.999
	Sample 3	0			0		
	Control 1	9.9 × 10 ⁵	0.0		9.9 × 10 ⁵	0.0	
	Control 2	8.1 × 10 ⁵	9.0 × 10 ⁵	-	8.1 × 10 ⁵	9.0 × 10 ⁵	-
120s	Sample 1	3.0 × 10 ¹			2.0 × 10 ¹		
	Sample 2	1.5 × 10 ¹	2.8 × 10 ¹	99.997	2.0 × 10 ¹	2.5 × 10 ¹	99.997
	Sample 3	4.0 × 10 ¹			3.5 × 10 ¹		
	Sample 1	0			0		
140s	Sample 2	0	0	99.999	0	0	99.999
	Sample 3	0			0		

Glass - Staphylococcus aureus

			130 cm		100 cm			
Repeat #2	Sample	Result	Average	Reduction rate (%)	Result	Average	Reduction rate (%)	
Positive	Control 1	2.7 × 10 ⁶			2.7 × 10 ⁶	2.3 × 10 ⁶		
control	Control 2	2.0 × 10 ⁶	2.3 × 10 ⁶		2.0 × 10 ⁶	2.3 × 10°	-	
	Sample 1	2.2 × 10 ²			1.4 × 10 ²			
60s	Sample 2	3.0 × 10 ¹	1.0 × 10 ²	99.996	1.7 × 10 ²	1.9 × 10²	99.992	
	Sample 3	5.5 × 10 ¹			2.7 × 10 ²			
	Sample 1	1.5 × 10 ²			4.0 × 10 ¹			
80s	Sample 2	1.6 × 10 ²	1.1 × 10 ²	99.995	1.5 × 10 ¹	5.7 × 10 ¹	99.998	
	Sample 3	3.5 × 10 ¹			1.2 × 10 ²			
	Sample 1	1.7 × 10 ²			2.5 × 10 ¹			
100s	Sample 2	1.0 × 10 ¹	6.0 × 10 ¹	99.997	1.0 × 10 ¹	5.0 × 10 ¹	99.998	
	Sample 3	0			1.2 × 10 ²			
	Control 1	1.3 × 10 ⁶	1.2 × 105		1.3 × 10 ⁶	1.2 × 105		
	Control 2	1.2 × 10 ⁶	1.2 × 10 ⁶	-	1.2 × 10 ⁶	1.2 × 10 ⁶	-	
120s	Sample 1	5.5 × 10 ¹			2.5 × 10 ¹			
	Sample 2	2.5 × 10 ¹	3.7 × 101	99.997	5.0 × 10º	1.5 × 10 ¹	99.998	
	Sample 3	3.0 × 10 ¹			1.5 × 10 ¹			
	Sample 1	0			0			
140s	Sample 2	0	2.0 × 10 ⁰	99.999	1.5 × 10 ¹	7.0 × 10º	99.999	
	Sample 3	5.0 × 10 ⁰			5.0 × 10 ⁰			

Glass - Staphylococcus aureus

			130 cm			100 cm	
Repeat #3	Sample	Result	Average	Reduction rate (%)	Result	Average	Reduction rate (%)
Positive	Control 1	2.2 × 10 ⁶	2.7 × 10 ⁶		2.2 × 10 ⁶	2.7 × 10 ⁶	
control	Control 2	3.3 × 10 ⁶	2.7 * 10°		3.3 × 10 ⁶	2.7 × 10°	-
	Sample 1	1.7 × 10 ²			1.0 × 10 ¹		
60s	Sample 2	9.0 × 10 ¹	1.4 × 10 ²	99.994	3.4 × 10 ²	1.5 × 10²	99.994
	Sample 3	1.5 × 10 ²			1.0 × 10 ²		
	Sample 1	2.7 × 10 ²			5.0 × 10 ⁰		
80s	Sample 2	1.0 × 10 ¹	1.2 × 10 ²	99.996	2.3 × 10 ²	8.7 × 10 ¹	99.997
	Sample 3	7.5 × 10 ¹	101		2.5 × 10 ¹		
	Sample 1	5.0×10^{0}			1.0 × 10 ¹		
100s	Sample 2	4.5 × 10 ¹	2.2 × 10 ¹	99.999	5.0 × 10 ¹	4.8×10^{1}	99.998
	Sample 3	1.5 × 10 ¹			8.5 × 10 ¹		
	Control 1	2.0 × 10 ⁶	2.0		2.0 × 10 ⁶	2.0	
	Control 2	2.0 × 10 ⁶	2.0 × 10 ⁶	-	2.0 × 10 ⁶	2.0 × 10 ⁶	-
120s	Sample 1	1.5 × 10 ¹			0		
	Sample 2	1.0 × 10 ¹	1.2 × 10 ¹	99.999	0	0	99.999
	Sample 3	1.0 × 10 ¹			0		
	Sample 1	0			0		
140s	Sample 2	0	5.0 × 10º	99.999	0	5.0 × 10º	99.999
	Sample 3	1.5 × 10 ¹			1.5 × 10 ¹		

Date: APR. 02, 2021

Glass - Salmonella enteritidis

			130 cm			100 cm	
Repeat #1	Sample	Result	Average	Reduction rate (%)	Result	Average	Reduction rate (%)
Positive	Control 1	1.0 × 10 ⁵			1.0 × 10 ⁵		
control	Control 2	9.8 × 10 ⁴	1.0 × 10 ⁵	-	9.8 × 10 ⁴	1.0 × 10 ⁵	-
	Sample 1	2.3 × 10 ²			9.5 × 10 ¹	1.1×10^{2}	
60s	Sample 2	1.8 × 10 ²	2.2 × 10 ²	99.780	6.0 × 10 ¹		99.890
	Sample 3	2.6 × 10 ²			1.7 × 10 ²		
	Sample 1	9.0 × 10 ¹			2.5 × 10 ¹		
80s	Sample 2	1.5 × 10 ¹	6.0 × 10 ¹	99.940	1.0 × 10 ¹	1.3 × 10 ¹	99.987
	Sample 3	7.5 × 10 ¹			5.0 × 10 ⁰		
	Sample 1	5.0 × 10 ⁰			0		
100s	Sample 2	5.0 × 10 ⁰	5.0 × 10 ⁰	99.995	0	2.0 × 10 ⁰	99.998
	Sample 3	5.0 × 10 ⁰			5.0 × 10 ⁰		
	Control 1	5.2 × 10 ⁵			5.2 × 10 ⁵		
	Control 2	5.7 × 10 ⁵	5.5 × 10⁵	_	5.7 × 10 ⁵	5.5 × 10⁵	-
120s	Sample 1	0	0	99.999	5.0 × 10 ⁰	1.7 × 10 ¹	
	Sample 2	0			2.0 × 10 ¹		99.996
	Sample 3	0			2.5 × 10 ¹		
	Sample 1	0			0		
140s	Sample 2	0	0	99.999	0	0	99.999
	Sample 3	0			0		
Positive	Control 1	-			4.4 × 10 ⁵	4.0 4.05	
control	Control 2	-	-	-	3.5 × 10⁵	4.0 × 10 ⁵	-
	Sample 1	-			5.0×10^{0}		
160s	Sample 2	-	-	-	0	2.0 × 10 ⁰	99.999
	Sample 3	-			0		
	Sample 1	-			5.0 × 10 ⁰		
180s	Sample 2	-	-	-	0	2.0 × 10 ⁰	99.999
	Sample 3	-			0		

Date: APR. 02, 2021

Glass - Salmonella enteritidis

			130 cm			100 cm	
Repeat #2	Sample	Result	Average	Reduction rate (%)	Result	Average	Reduction rate (%)
Positive	Control 1	8.8 × 10 ⁵			8.8 × 10 ⁵		
control	Control 2	8.2 × 10 ⁴	8.5 × 10 ⁵	-	8.2 × 10 ⁴	8.5 × 10 ⁵	-
	Sample 1	1.1 × 10 ²		99.994	6.5 × 10 ¹	7.3 × 10 ¹	
60s	Sample 2	3.5 × 10 ¹	5.0 × 10 ¹		1.5 × 10 ²		99.991
	Sample 3	5.0 × 10 ⁰			1.0 × 10 ¹		
	Sample 1	4.5 × 10 ¹			1.5 × 10 ¹		
80s	Sample 2	0	1.7 × 10 ¹	99.998	4.5 × 10 ¹	2.3 × 10 ¹	99.997
	Sample 3	5.0 × 10 ⁰			1.0 × 10 ¹		
	Sample 1	0			0		
100s	Sample 2	0	0	99.999	5.0 × 10 ⁰	3.0 × 10 ⁰	99.999
	Sample 3	0			5.0 × 10 ⁰		
	Control 1	5.4 × 10 ⁵			5.4 × 10 ⁵	5.7 × 10 ⁵	
	Control 2	6.0 × 10 ⁵	5.7 × 10 ⁵	-	6.0 × 10 ⁵		-
120s	Sample 1	1.0 × 10 ²	0	99.997	5.0×10^{0}	1.0 × 10 ¹	
	Sample 2	2.5 × 10 ¹			2.5 × 10 ¹		99.998
	Sample 3	1.0 × 10 ¹			0		
	Sample 1	0			0		
140s	Sample 2	0	0	99.999	0	5.0 × 10 ⁰	99.999
	Sample 3	0			5.0 × 10 ⁰		
Positive	Control 1	-			3.8 × 10 ⁵		
control	Control 2	-	-	-	4.7 × 10 ⁵	4.3 × 10 ⁵	-
	Sample 1	-			5.0 × 10 ⁰		
160s	Sample 2	-	-	-	0	2.0 × 10 ⁰	99.999
	Sample 3	-			0		
	Sample 1	-			1.0 × 10 ¹		99.999
180s	Sample 2	-	-	-	0	3.0 × 10 ⁰	
	Sample 3	-			0		

Date: APR. 02, 2021

Glass - Salmonella enteritidis

			130 cm			100 cm	
Repeat #3	Sample	Result	Average	Reduction rate (%)	Result	Average	Reduction rate (%)
Positive	Control 1	1.4 × 10 ⁵			1.4 × 10 ⁵		
control	Control 2	2.1 × 10 ⁴	1.7 × 10 ⁵	-	2.1 × 10 ⁴	1.7 × 10 ⁵	-
	Sample 1	1.0 × 10 ¹			8.0 × 10 ¹		
60s	Sample 2	1.5 × 10 ¹	4.2 × 10 ¹	99.975	5.0 × 10 ⁰	3.8 × 10 ¹	99.978
	Sample 3	1.0 × 10 ²			3.0 × 10 ¹		
	Sample 1	1.0 × 10 ¹			0		
80s	Sample 2	0	1.3 × 10 ¹	99.992	0	2.0 × 10 ⁰	99.998
	Sample 3	3.0 × 10 ¹			5.0 × 10 ⁰		
	Sample 1	0			6.0 × 10 ¹		
100s	Sample 2	1.0 × 10 ¹	8.0×10^{0}	99.997	2.5 × 10 ¹	3.2 × 10 ¹	99.981
	Sample 3	1.5 × 10 ¹			1.0 × 10 ¹		
	Control 1	2.3 × 10 ⁶			2.3 × 10 ⁶	2.3 × 10 ⁶	
	Control 2	2.2 × 10 ⁶	2.3 × 10 ⁶	-	2.2 × 10 ⁶		-
120s	Sample 1	0	1.2×10^{1}		2.0 × 10 ¹		
	Sample 2	2.0 × 10 ¹		99.999	2.0 × 10 ¹	1.3×10^{1}	99.999
	Sample 3	1.5 × 10 ¹			0		
	Sample 1	0			0		
140s	Sample 2	0	0	99.999	0	5.0×10^{0}	99.998
	Sample 3	0			5.0×10^{0}		
Positive	Control 1	-			3.8 × 10 ⁵	F 0 + 105	
control	Control 2	-	-	-	6.1 × 10 ⁵	5.0 × 10 ⁵	-
	Sample 1	-			5.0 × 10 ⁰		
160s	Sample 2	-	-	-		3.0 × 10 ⁰	99.999
	Sample 3	-			5.0 × 10 ⁰		
	Sample 1	-			0		
180s	Sample 2	-	-	-	0	0	99.999
	Sample 3	-			0		

Date: APR. 02, 2021

Fabric - Staphylococcus aureus

			130 cm			100 cm	
Repeat #1	Sample	Result	Average	Reduction rate (%)	Result	Average	Reduction rate (%)
Positive	Control 1	3.7 × 10⁵	4.0 × 10 ⁵	-	3.7 × 10⁵	4.0 × 10 ⁵	_
control	Control 2	4.3 × 10 ⁵	4.0 × 10 ³	-	4.3 × 10 ⁵	4.0 × 10 ³	-
	Sample 1	1.5 × 10 ¹			5.0 × 10 ⁰		
60s	Sample 2	0	5.0 × 10 ⁰	99.998	5.0 × 10 ⁰	3.0×10^{0}	99.999
S	Sample 3	0			0		
	Sample 1	0			0		
80s	Sample 2	0	0	99.999	0	0	99.999
	Sample 3	0			0		
	Sample 1	0		99.999	0	0	99.999
100s	Sample 2	5.0 × 10 ⁰	2.0 × 10 ⁰		0		
	Sample 3	0			0		
	Sample 1	0			0		
120s	Sample 2	5.0 × 10º	2.0 × 10 ⁰	99.999	0	0	99.999
	Sample 3	0			0		
	Sample 1	0			5.0×10^{0}		
140s	Sample 2	0	0	99.999	0	3.0 × 10 ⁰	99.999
	Sample 3	0			5.0 × 10 ⁰		

Fabric - Staphylococcus aureus

			130 cm			100 cm	
Repeat #2	Sample	Result	Average	Reduction rate (%)	Result	Average	Reduction rate (%)
Positive	Control 1	8.1 × 10 ⁶	7.0 × 106		8.1 × 10 ⁶	7.0 × 106	
control	Control 2	6.4 × 10 ⁶	7.2 × 10 ⁶		6.4 × 10 ⁶	7.2 × 10 ⁶	-
	Sample 1	5.0 × 10 ⁰			0		
60s	Sample 2	0	2.0 × 10 ⁰	99.999	2.0 × 10 ¹	1.5 × 10 ¹	99.999
	Sample 3	0			2.5 × 10 ¹		
	Sample 1	1.0 × 10 ¹			1.0×10^{1}		
80s	Sample 2	5.0 × 10 ⁰	8.0×10^{0}	99.999	2.0 × 10 ¹	1.2 × 10 ¹	99.999
	Sample 3	1.0 × 10 ¹			5.0×10^{0}		
	Sample 1	5.0 × 10 ⁰			5.0×10^{0}		
100s	Sample 2	0	3.0×10^{0}	99.999	0	3.0×10^{0}	99.999
	Sample 3	5.0 × 10º			5.0 × 10º		
	Control 1	7.3 × 10 ⁵	F 0 105		7.3 × 10 ⁵	F 0 ··· 405	
	Control 2	4.4 × 10 ⁵	5.8 × 10 ⁵	-	4.4 × 10 ⁵	5.8 × 10 ⁵	-
120s	Sample 1	5.0 × 10 ⁰			0		
	Sample 2	0	2.0 × 10 ⁰	99.999	5.0 × 10 ⁰	2.0 × 10 ⁰	99.999
	Sample 3	0			0		
	Sample 1	5.0 × 10 ⁰			0		
140s	Sample 2	5.0 × 10 ⁰	5.0 × 10 ⁰	99.999	5.0×10^{0}	2.0×10^{0}	99.999
	Sample 3	5.0 × 10 ⁰			0		

Fabric - Staphylococcus aureus

		130 cm			100 cm		
Repeat #3	Sample	Result	Average	Reduction rate (%)	Result	Average	Reduction rate (%)
Positive control	Control 1	3.9 × 10 ⁵	5.6 × 10 ⁵	-	3.9 × 10 ⁵	5.6 × 10⁵	-
	Control 2	7.4 × 10 ⁵			7.4 × 10 ⁵		
	Sample 1	0		99.999	1.0 × 10 ¹	5.0 × 10 ⁰	99.999
60s	Sample 2	0	5.0 × 10 ⁰		0		
	Sample 3	1.5 × 10 ¹			5.0 × 10 ⁰		
	Sample 1	1.0 × 10 ¹	3.0 × 10 ⁰	99.999	5.0 × 10 ⁰	2.0 × 10 ⁰	99.999
80s	Sample 2	0			0		
	Sample 3	0			0		
100s	Sample 1	5.0 × 10 ⁰	2.0 × 10 ⁰	99.999	0	0	99.999
	Sample 2	0			0		
	Sample 3	0			0		
	Control 1	8.1 × 10 ⁵	- 8.3 × 10 ⁵	-	8.1 × 10 ⁵	8.3 × 10 ⁵	-
	Control 2	8.6 × 10 ⁵			8.6 × 10 ⁵		
120s	Sample 1	0	0	99.999	2.5 × 10 ¹	1.0 × 101	99.998
	Sample 2	0			5.0 × 10º		
	Sample 3	0			0		
140s	Sample 1	0	0		5.0 × 10 ⁰	5.0 × 10º	99.999
	Sample 2	0		99.999	1.0 × 10 ¹		
	Sample 3	0			0		

Fabric - Klebsiella pneumoniae

Repeat #1		130 cm			100 cm		
	Sample	Result	Average	Reduction rate (%)	Result	Average	Reduction rate (%)
Positive control	Control 1	1.0 × 107	9.5 × 10 ⁶	-	1.0 × 107	9.5×10^{6}	-
	Control 2	8.9 × 10 ⁶			8.9 × 10 ⁶		
	Sample 1	0		99.999	0	2.0 × 10 ⁰	99.999
60s	Sample 2	0	0		0		
	Sample 3	0			5.0×10^{0}		
	Sample 1	8.5 × 10 ¹	8.8 × 10 ¹	99.999	2.0 × 10 ¹	8.2 × 10 ¹	99.999
80s	Sample 2	2.5 × 10 ¹			1.6 × 10 ²		
	Sample 3	1.6 × 10 ²			7.5 × 10 ¹		
100s	Sample 1	0	5.0 × 10 ⁰	99.999	5.0×10^{0}	1.7 × 10 ¹	99.999
	Sample 2	5.0 × 10 ⁰			0		
	Sample 3	1.0 × 10 ¹			4.5 × 10 ¹		
	Control 1	3.8 × 10 ⁶	- 3.6 × 10 ⁶	-	3.8 × 10 ⁶	3.6×10^{6}	-
	Control 2	3.3 × 10 ⁶			3.3 × 10 ⁶		
120s	Sample 1	0			0		
	Sample 2	0	0	99.999	0	0	99.999
	Sample 3	0			0		
140s	Sample 1	5.0 × 10 ⁰	2.0 × 10 ⁰		0	3.0 × 10 ⁰	
	Sample 2	0		99.999	5.0×10^{0}		99.999
	Sample 3	0			5.0 × 10 ⁰		

Fabric - Klebsiella pneumoniae

Repeat #2		130 cm			100 cm		
	Sample	Result	Average	Reduction rate (%)	Result	Average	Reduction rate (%)
Positive control	Control 1	4.5 × 10 ⁶	4.0 × 10 ⁶		4.5 × 10 ⁶	4.0 × 10 ⁶	-
	Control 2	3.6 × 10 ⁶			3.6 × 10 ⁶		
	Sample 1	1.5 × 10 ¹		99.999	1.5 × 10 ¹	7.0 × 10 ⁰	99.999
60s	Sample 2	1.5 × 10 ¹	1.3 × 10 ¹		5.0×10^{0}		
	Sample 3	1.0 × 10 ¹			0		
	Sample 1	0		99.999	0	2.0 × 10 ⁰	99.999
80s	Sample 2	0	0		0		
	Sample 3	0			5.0 × 10 ⁰		
	Sample 1	0	3.0 × 10 ⁰	99.999	1.0 × 10 ¹	1.2 × 10 ¹	99.999
100s	Sample 2	5.0 × 10 ⁰			1.0 × 10 ¹		
	Sample 3	5.0 × 10 ⁰			1.5 × 10 ¹		
	Control 1	2.5 × 10 ⁶	- 2.3 × 10 ⁶	-	2.5 × 10 ⁶	- 2.3 × 10 ⁶	-
	Control 2	2.1 × 10 ⁶			2.1 × 10 ⁶		
120s	Sample 1	1.0 × 10 ¹	5.0 × 10º	99.999	0	0	99.999
	Sample 2	5.0 × 10 ⁰			0		
	Sample 3	0			0		
140s	Sample 1	5.0 × 10 ⁰	5.0 × 10 ⁰		1.0×10^{1}	7.0 × 10 ⁰	99.999
	Sample 2	5.0 × 10 ⁰		99.999	5.0 × 10 ⁰		
	Sample 3	5.0 × 10 ⁰			5.0×10^{0}		

Fabric - Klebsiella pneumoniae

Repeat #3		130 cm			100 cm		
	Sample	Result	Average	Reduction rate (%)	Result	Average	Reduction rate (%)
Positive control	Control 1	5.5 × 10 ⁶	6.1×10^{6}	-	5.5 × 10 ⁶	6.1 × 10 ⁶	-
	Control 2	6.8 × 10 ⁶			6.8 × 10 ⁶		
	Sample 1	5.0 × 10 ⁰		99.999	1.5 × 10 ¹	1.3 × 10 ¹	99.999
60s	Sample 2	0	7.0×10^{0}		1.0 × 10 ¹		
	Sample 3	1.5 × 10 ¹			1.5 × 10 ¹		
	Sample 1	0	0	99.999	0	3.0 × 10 ⁰	99.999
80s	Sample 2	0			5.0×10^{0}		
	Sample 3	0			5.0×10^{0}		
100s	Sample 1	0	0	99.999	5.0×10^{0}	5.0 × 10 ⁰	99.999
	Sample 2	0			1.0 × 10 ¹		
	Sample 3	0			0		
	Control 1	6.7 × 10 ⁶	6.1 × 10 ⁶	-	6.7 × 10 ⁶	6.1 × 10 ⁶	-
	Control 2	5.6 × 10 ⁶			5.6 × 10 ⁶		
120s	Sample 1	0	0	99.999	0	0	99.999
	Sample 2	0			0		
	Sample 3	0			0		
140s	Sample 1	5.0 × 10 ⁰	5.0 × 10º		0	2.0 × 10 ⁰	99.999
	Sample 2	0		99.999	0		
	Sample 3	1.0 × 10 ¹			5.0×10^{0}		

SECTION 11

Conclusion

Based on the data collected the Hypothesis is accepted:

Staphylococcus aureus on stainless steel & glass exposed to UVC lamp at a distance of 1 M can decreased 99.999% at more than 140 seconds.

Salmonella on stainless steel & glass exposed to UVC lamp at a distance of 1 M can decreased 99.999% at more than 160 seconds.


Staphylococcus aureus & Klebsiella pneumoniae on fabric exposed to UVC lamp at a distance of 1 M can decreased 99.999% at more than 140 seconds.

Date: APR. 02, 2021

APPEXDIX I. Photos of sample



<Front view>

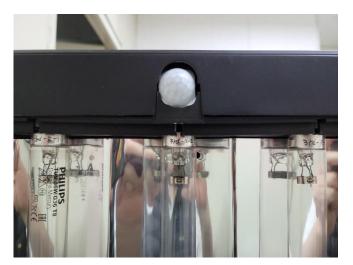

<Lamp position view>